



Available online at
ScienceDirect
www.sciencedirect.com

Elsevier Masson France
EM|consulte
www.em-consulte.com/en



Original article

Pressure algometry is a useful tool to quantify pain in the medial part of the knee: An intra- and inter-reliability study in healthy subjects



X. Pelfort^a, R. Torres-Claramunt^{b,*}, J.F. Sánchez-Soler^b, P. Hinarejos^{b,c}, J. Leal-Blanquet^b, D. Valverde^d, J.C. Monllau^{b,c}

^a Orthopaedic department, Consorci Sanitari de l'Ànoia, Avinguda Catalunya 11, 08700 Igualada, Barcelona, Spain

^b Orthopaedic department, Hospital del Mar, Universitat Autònoma de Barcelona, Passeig Marítim 25–29, 08003 Barcelona, Spain

^c IMIM, Hospital del Mar Medical Research Institute, Barcelona, Spain

^d Orthopaedic department, Hospital General de Granollers, Universitat Internacional de Catalunya, Granollers, Barcelona, Spain

ARTICLE INFO

Article history:

Received 14 December 2014

Accepted 2 March 2015

Keywords:

Algometry
 Pressure
 Pain
 Knee
 Threshold

ABSTRACT

Purpose: Pain quantification is essential for diagnostic and pain monitoring purposes in disorders around the knee. Pressure algometry is a method described to determine pressure pain threshold (PPT) by applying controlled pressure to a given body point. The purpose of this study was to determine the reliability of this method when it was applied to the medial part of the proximal tibia metaphysis and to evaluate the PPT levels between genders.

Methods: Fifty healthy (mean age; 46.9) volunteers were recruited, 25 men and 25 women. Pressure algometry was applied to a 1 cm²-probe area on the medial part of the knee by 2 raters. Intra- and inter-class correlation (ICC) was obtained and differences between genders were evaluated. Bland-Altman plots were performed to evaluate the variability of the measures.

Results: The mean values of PPT obtained by rater 1 and 2 were 497.5 Kpa and 489 Kpa respectively. The intrarater reliability values (95% IC) for rater 1 and 2 were 0.97 (0.95–0.98) and 0.84 (0.73–0.90) respectively. With regard to interrater reliability, the ICC (95% IC) for the first measurement was 0.92 (0.87–0.95) and 0.86 (0.78–0.92) for the second one. Women showed significant lower values of PPT than men. The Bland-Altman plots showed excellent agreement.

Conclusions: Pressure algometry has excellent reliability when it is applied to the medial part of the proximal metaphysis of the tibia. Women have lower values of PPT than men. The high reliability of the PA in an individual volunteer makes it a more valuable tool for longitudinal assessment of a given patient than for comparison between them.

Level of evidence: Level III. Prospective study.

© 2015 Elsevier Masson SAS. All rights reserved.

1. Introduction

Quantification of the pain is essential for diagnostic and pain monitoring purposes. Tenderness is the major symptom of muscle-skeletal dysfunction and its accurate evaluation is important in the diagnostic procedure. In the clinical practice, digital pressure palpation is normally used to locate and assess the pain. However, this method is difficult to quantify and standardize because of the different degrees of pressure applied by the same or different examiners as well as the subjective report of pain by the patient [1].

The Pressure Pain Threshold (PPT) is defined as the point at which a non-painful pressure stimulus turns into a painful pressure

sensation. Pressure algometry (PA) is a method described to objectively quantify this PPT. This technique is a well-known and well-validated method to induce acute experimental pain. Different studies have been published about using this tool to evaluate pain in different locations of the body and showed high levels of reliability. Furthermore, some other studies concluded that PA is a worthwhile tool in the diagnosis and treatment evaluation of different orthopaedic disorders [1–7].

With regard on the different orthopaedic procedures that can be applied to an arthritic or pre-arthritic knee, these are conditioned by objective data (radiology and different scores; WOMAC, KSS or Oxford score. . .) as well as the pain referred. Until now, the most objective tool and the gold standard method to quantify the pain is the Visual Analogue Scale (VAS). This score is very subjective depending on the patient and a high correlation with the PPT has been observed in a previous study [8]. Nevertheless, it has been

* Corresponding author.

E-mail address: rtorresclaramunt@parcdesalutmar.cat (R. Torres-Claramunt).

used by other authors for pre- and postoperative evaluation of pain at the medial side of the knee in patients undergoing valgus tibial osteotomy [9–13]. Given the need to better improve the method to quantify the tenderness, not only to consider the more accurate surgical option but also to monitor the pain [14,15], it was considered the possibility to apply the PA in the knee orthopaedic disorders.

The main objective of this study was to determine in healthy volunteers the reliability of PA when it was applied on the medial part of the proximal tibia metaphysis. A second objective was to evaluate if there were differences in PPT at the medial side of the knee between men and women. Our hypothesis was that PA is a reliable tool to quantify the pain.

2. Material and methods

Fifty healthy volunteers were recruited for this study. The inclusion criteria were: age ranging from 25 to 65 years, no history of lower limb, spine or pelvic fractures, the absence of skin disorders, peripheral neuropathies or vascular diseases. Patients who took painkillers for any reason in the previous week were also excluded. All volunteers were Caucasian and the mean age was 46.9 (28–63). The experimental procedure was explained and signed informed consent was obtained from each participant. The study was approved by the ethics committee of our institution with the registry number 2013/5058/I.

PPT was determined using a handheld electronic pressure algometer with a 1 cm² probe area with an increasing of the pressure rate of 20 Kpa/s (Algometer, Somedic Sales, Hörby, Sweden). The pressure algometer consists of a “pistol” handle and a rod with a pressure-sensitive gauge strain at the tip. All the measurements were performed at 1 cm distal from the medial knee joint line with the knee flexed at 90° (Fig. 1). This location was chosen because it is the point usually used to evaluate the presence of pain in the medial part of the knee when considering a surgical procedure like a unicompartimental or total knee arthroplasty or a high tibial osteotomy.

PA was performed on the same day under quiet and non-stressful conditions. The tip of the algometer was positioned on this specific point. By pushing the algometer, the force applied to the tibia gradually increased. The participants were not allowed to see the algometer display in any moment, and, as soon as the

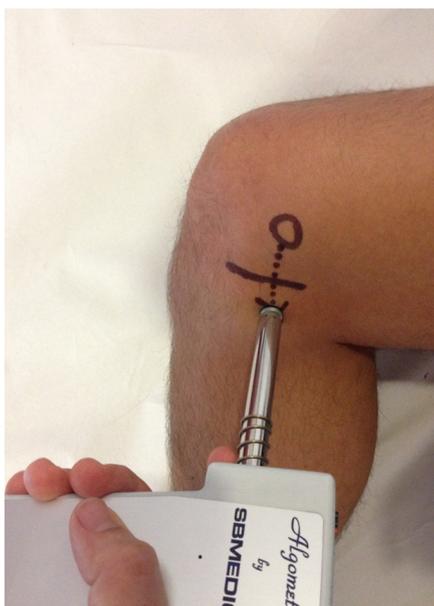


Fig. 1. Algometry measurement procedure, location and method of use.

Table 1
Epidemiological data and measurements description.

Number of participants	50
Male:Female	25:25
Mean age (range)	46.9 (28–63)
Standard deviation	10.7
Number of measurements taken by each observer each time	3
Interval between measurements for a single observer (minutes)	1
Interval between measurements per participant (minutes)	15
Interval between two measurements (hours)	4.5
Total of measurements per participant	12
Total of measurements per observer	300

volunteers experienced a painful sensation, they said “stop”, the algometer was immediately released and the force (in Kpa) was read from the display.

Two trained raters were instructed in the application of algometry. To determine the value of PPT, we used the method described by Nussbaum and Downes [16]. Both raters made 3 consecutive algometry applications at the prescribed rate of 20 KPa/s, 1 minute apart. The first measurement was considered as a trial and the final value of the PPT was calculated from the mean of the second and third measurements. The number of raters (2), the time elapsed between both measurements (3–4 hours) and the time between measurements per participant (10–20 minutes) were decided on with the purpose properly evaluating the device and avoiding potential disturbances of any clinical variation of the patient between measurements [1,17]. The protocol is summarized in Fig. 2. Epidemiological data and measurements descriptions are shown in Table 1.

2.1. Statistical analysis

Descriptive statistics was used for demographic data. The intra- and interclass coefficient correlation (ICC) values were assessed. In order to identify the precision of the estimate, the 95% of confidence interval (IC) was assessed. The ICC values were classified as follows: <0.4 indicated poor agreement; 0.4 to 0.75, moderate agreement; and >0.75, excellent agreement [18,19]. Systematic error evaluation between measurements, raters and gender was assessed with paired the Student's *t* test [20,21]. *P*-values less than 0.05 were considered statistically significant. Bland-Altman plots were performed in which differences between two consecutive PPT measurements and between the two raters were graphically represented [22]. All analysis and plots were performed with R3.0 (The R project for statistical computing).

3. Results

Fifty volunteers were finally assessed, 25 men and 25 women, with a mean age of 46.9 years (range 28–63, SD 10.7) (Table 1). Pressure algometry was well-tolerated by all the participants. The mean PPT obtained by the rater 1 and 2 was 497.5 Kpa and 489.0 Kpa respectively. The mean PPT obtained in the first measurement was 497.5 Kpa and in the second one, 505.9 Kpa. The ICC values for both, inter- and intra-rater reliability, was excellent give the ICC value (Tables 2 and 3). Women showed significant lower values of PPT than men with mean values of PPT 387 Kpa and 616.2 Kpa respectively (Table 4). All values showed in Tables 2–4 presented an excellent correlation with the exception of women for the second measurement or when women were evaluated by the rater 2 (moderate correlation).

The values of the systematic error of evaluation translate the differences between both measurements for each volunteer. This systematic error was measured as mean and standard deviation. The fact that all *P*-values of the systematic error of evaluation were not significant (*P*>0.05) means that there was an absence of a

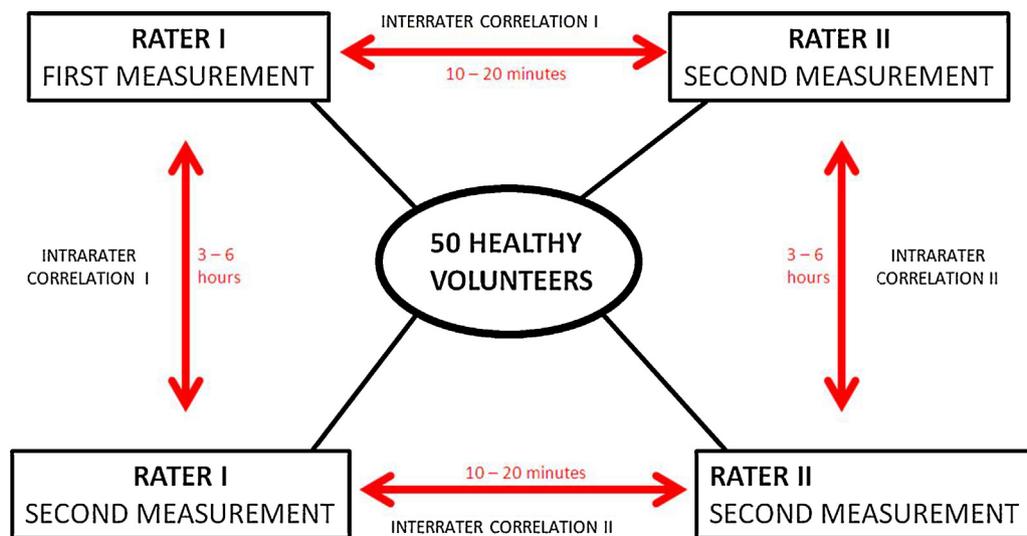


Fig. 2. Protocol of measurements for both raters.

Table 2

Intra-rater agreement values.

Intra-rater	Agreement ICC (95% CI)	Mean	SD	Systematic error evaluation	
				Mean	SD
Rater 1	0.97 (0.95–0.98)	497.5	201.8	–8.4	47.1
Rater 2	0.84 (0.73–0.90)	489.0	206.4	–3.8	117.2

Mean: mean difference, in Kpa, between the first and second measurements (intra-rater); SD: standard deviation of the mean differences.

Table 3

Inter-rater agreement values.

Inter-rater	Agreement ICC (95% CI)	Mean	SD	Systematic error evaluation	
				Mean	SD
Measurement 1	0.92 (0.87–0.95)	497.5	212.2	8.4	80.1
Measurement 2	0.86 (0.73–0.9)	505.9	203.4	13.1	104.9

Mean: mean difference, in Kpa, between the first and second measurements (intra-rater); SD: standard deviation of the mean differences.

Table 4

Inter and intra-rater agreement values for both raters and both measurements divided on men and women.

Inter-rater correlation			Intra-rater correlation		
First measurement	ICC (95% CI)	Mean (Kpa)	Rater 1	ICC (95%)	Mean (Kpa)
Men	0.92 (0.82–0.96)	614.6	Men	0.95 (0.89–0.97)	614.6
Women	0.86 (0.72–0.93)	380.3	Women	0.98 (0.94–0.99)	380.3 ^a
Second measurement			Rater 2		
Men	0.86 (0.71–0.93)	617.9	Men	0.89 (0.77–0.95)	580.4
Women	0.68 (0.40–0.84)	394.0	Women	0.55 (0.20–0.77)	397.6

^a $P < 0.05$.

systematic error in these measurements. Only in one measurement in Table 4, the P -value obtained was < 0.05 .

The Bland-Altman plots for all the evaluations are included in the Fig. 3 and illustrated the distribution of the different algometry values. This PPT ranged from 200 to 900 Kpa/cm² and it was found an excellent intra- and inter-rater agreement.

4. Discussion

The main finding of this study was that PA has an excellent inter- and intra-rater reliability when the PPT is measured on the medial part of the proximal metaphysis of the tibia. Based on this, the hypothesis has been confirmed. These results confirmed that algometry might be a useful tool in objectifying pain in this part

of the knee. Secondly, it was observed a higher PPT values for men. Different authors have studied the utility of this technique in different parts of the body. They concluded that the PA has a good agreement between observers. Farasyn et al. [23] studied the applicability of this method in patients with non-specific low back pain by applying a deep cross-friction pressure in the proximal gluteus region. They observed excellent inter- (ICC 0.97) and intra-rater (ICC 0.98) reliability. Other authors also showed a good reliability for this technique in other parts of the body; the first dorsal interosseous muscle [1], the neck and head muscles [4,6,7,17,24] or following a spinal manipulation [25].

Different studies have assessed the utility of PA with different disorders involving soft tissues of the knee. Van Wilgen et al. [5] studied the reliability of this instrument in athletes with patellar

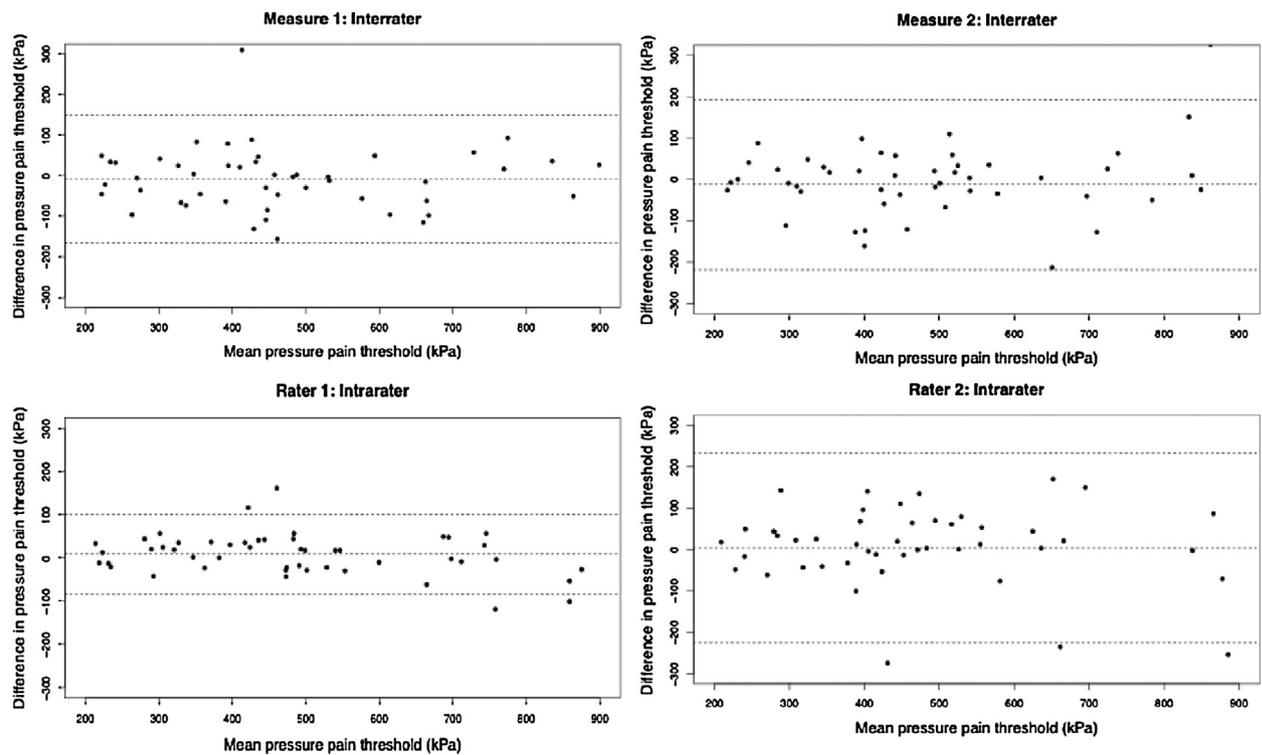


Fig. 3. Bland-Altman plots shows distribution of data of each measurement and rater data.

tendinopathy. They observed that the PTT of asymptomatic athletes differed from that of athletes with tendinopathy and showed excellent inter-rater (ICC 0.93) and moderate intra-rater (ICC 0.6) reliability. In this study, the authors placed the algometer on the distal apex of the patella for the control group and directly on the most painful spot of the patellar tendon in the group with tendinopathy. In a similar way, other authors evaluated the potential usefulness of the PA as a tool to evaluate and monitoring the clinical evolution of the pain at the medial side of the tibia in runners who suffered a tibial stress syndrome. They also found lower values of PPT in this specific population compared to a healthy group of volunteers and concluded that PA may be a useful tool to evaluate this painful syndrome [26]. On the other hand, Lunn et al. [27] assessed the PPT levels in patients who had undergone a total knee arthroplasty. They observed significant higher PPT values during quadriceps contraction compared when the muscle was relaxed. It is a well-known phenomenon that active muscle contraction may increase the local value of the PPT [28,29].

In the study here presented, all measures were performed in a non-stressful condition and in a location (proximal metaphysis of the tibia) without any muscle disturbance. The 1-cm distal to the joint line is the one where we usually apply digital pressure to reproduce pain in the medial compartment of the knee in pre-arthritic or arthritic knees.

Our hypothesis is confirmed and the PA could be thus routinely applied in the decision-making protocol of the different therapeutic options around the knee.

Another interesting finding of this study was the significant lower values of PPT obtained in women compared with men. Previous studies have found similar results when PA was applied in other locations of the human body [30,31]. Fisher et al., in a study, conducted in a healthy population found higher values of PPT in males in 8 out of 9 different muscle regions evaluated [32]. In a recent study, Aweid et al. [26] analyzed the PTT in healthy runners in the medial part of the distal tibia. They also observed a lower PTT in females compared to males. The reasons to explain these

findings are not well-known, but different authors referred hormonal reasons as a possible explanation for these differences [33,34].

The mean values obtained by the 2 raters ranged around 500 Kpa with a mean standard deviation around 200 Kpa. These results mean that exist an important variability of the PPT for the different healthy volunteers. However, the low values of the systematic error measurement, mean that, despite this variability of the PTT between the volunteers, these values are constant for the same volunteer, independently of the number of measurements done or the rater involved in the measurement. This tool may thus be more useful in monitoring pain in a patient before/after a given procedure than comparing patients between them.

The algometer used in this study requires that the observer see the digital display during the measurement in order to increase the local pressure while maintaining a constant speed (20 Kpa/s). This fact means that the final value (in Kpa) is determined when the volunteer say "stop", but this value is not blinded for the rater. This fact may be considered as a limitation of this study. Moreover, although this study only considered healthy volunteers and the correlation between VAS and PA has been studied in a previous work [8], the fact of not comparing these 2 scores between them in this study could be considered as another limitation.

5. Conclusions

Pressure algometry has excellent intra- and interrater agreement when is applied on the medial part of the tibial metaphysis in a healthy subject. Women have a lower PTT levels at this location than men. The high reliability of the PA in an individual volunteer makes it a more valuable tool for longitudinal assessment of a given patient than for comparison between patients.

Disclosure of interest

The authors declare that they have no conflicts of interest concerning this article.

Acknowledgment

The authors thank Sergi Mojal from MCBR (methodological consulting in biomedical research) for his assistance in the statistical analysis of this work. We are also grateful to Eric Goode for his help in correcting the manuscript.

References

- [1] Chesterton LS, Sim J, Wright CC, Foster NE. Interrater reliability of algometry in measuring pressure pain thresholds in healthy humans, using multiple raters. *Clin J Pain* 2007;33:760–6.
- [2] Kosek E, Ekholm J, Hansson P. Pressure pain thresholds in different tissues in one body region. The influence of skin sensitivity in pressure algometry. *Scand J Rehab Med* 1999;31:89–93.
- [3] Fredberg U, Bolvig L, Pfeiffer-Jensen M, Clemmensen D, Jakobsen BW, Stengaard-Pedersen K. Ultrasonography as a tool for diagnosis, guidance of local steroid injection and, together with pressure algometry, monitoring of the treatment of athletes with chronic jumper's knee and Achilles tendinitis: a randomized, double-blind, placebo-controlled study. *Scand J Rheumatol* 2004;33:94–101.
- [4] Ylinen J, Nykänen M, Kautiainen H, Häkkinen A. Evaluation of repeatability of pressure algometry on the neck muscles for clinical use. *Man Ther* 2007;12:192–7.
- [5] Van Wilgen P, van der Noord R, Zwerver J. Feasibility and reliability of pain pressure threshold measurements in patellar tendinopathy. *J Sci Med Sport* 2011;14:477–81.
- [6] Walton D, Macdermid J, Nielson W, Teasell R, Chiasson M, Brown L. Reliability, standard error, and minimum detectable change of clinical pressure pain threshold testing in people with and without acute neck pain. *J Orthop Sports Phys Ther* 2011;41:644–50.
- [7] Walton D, Macdermid J, Nielson W, Teasell R, Nailor T, Maheu P. A descriptive study of pressure pain threshold at 2 standardized sites in people with acute or subacute neck pain. *J Orthop Sports Phys Ther* 2011;41:651–7.
- [8] Pelfort X, Güerri RC, Sánchez JF, Dürsteler C, Valverde D, Hinarejos P, et al. Bone micro-indentation and pressure algometry applied to revision total knee replacement and tibial end-of-stem pain. Preliminary results in a group of 20 patients. *Rev Esp Cir Orthop Traumatol* 2014;58:206–11.
- [9] El-Azab H, Morgenstern M, Ahrens P, Schuster T, Imhoff A, Lorenz G. Limb alignment after open-wedge high tibial osteotomy and its effect on the clinical outcome. *Orthopedics* 2011;34:622–8.
- [10] Zaffagnini S, Bonanzinga T, Grassi A, Muccioli G, Musiani C, Raggi F, et al. Combined ACL reconstruction and closing-wedge HTO for varus angulated ACL-deficient knees. *Knee Surg Sports Traumatol Arthrosc* 2013;21:934–41.
- [11] Kohn L, Sauerschnig M, Iskandar S, Lorenz S, Meidinger G, Imhoff AB, et al. Age does not influence the clinical outcome after high tibial osteotomy. *Knee Surg Sports Traumatol Arthrosc* 2013;21:146–51.
- [12] Bonasia D, Dettoni F, Sito G, Blonna D, Marmotti A, Bruzzone M, et al. Medial opening wedge high tibial osteotomy for medial compartment overload/arthritis in the varus knee. *Am J Sports Med* 2014;42:690–8.
- [13] Minzlaff P, Saier T, Brucker P, Haller B, Imhoff A, Hinterwimmer S. Valgus bracing in symptomatic varus malalignment for testing the expectable “unloading effect” following valgus high tibial osteotomy. *Knee Surg Sports Traumatol Arthrosc* 2014;17 [epub ahead of print].
- [14] Cobos R, Latorre A, Aizpuru F, Guenaga JI, Sarasqueta C, Escobar A, et al. Variability of indication criteria in knee and hip replacement: an observational study. *BMC Musculoskelet Disord* 2010;26(11):249.
- [15] Gossec L, Paternotte S, Maillefert JF, Combescure C, Conaghan PG, Davis AM, et al. OARSI-OMERACT Task Force “total articular replacement as outcome measure in OA”. The role of pain and functional impairment in the decision to recommend total joint replacement in hip and knee osteoarthritis: an international cross-sectional study of 1909 patients. Report of the OARSI-OMERACT Task Force on total joint replacement. *Osteoarthritis Cartilage* 2011;19:147–54.
- [16] Nussbaum E, Downes L. Reliability of clinical pressure-pain algometric measurements obtained on consecutive days. *Phys Ther* 1998;78:160–9.
- [17] Antonaci F, Sand T, Lucas G. Pressure algometry in healthy subjects: inter-examiner variability. *Scand J Rehab Med* 1998;30:3–8.
- [18] Shrout PE, Fleiss JL. Intraclass correlation: uses in assessing rater reliability. *Psychol Bull* 1979;86:420–8.
- [19] Fleiss JL, Levin B, Paik MC. Statistical methods for rates and proportions. Hoboken, New Jersey: John Wiley & Sons, Inc; 2003.
- [20] Weir JP. Quantifying test-retest reliability using the intraclass correlation coefficient and the SEM. *J Strength Cond Res* 2005;19:231e40.
- [21] Haley SM, Fragala-Pinkham MA. Interpreting change scores of tests and measures used in physical therapy. *Phys Ther* 2006;86:735–43.
- [22] Bland JM, Altman DG. Measuring agreement in method comparison studies. *Stat Methods Med Res* 1999;346:135–60.
- [23] Farasyn A, Meeusen R, Nijs J. Validity of cross-friction algometry procedure in referred muscle pain syndromes. *Clin J Pain* 2008;24:456–62.
- [24] Grossi DB, Chaves TC, Gonçalves MC, Moreira VC, Canonica AC, Florencio LL, et al. Pressure pain threshold in the craniocervical muscles of women with episodic and chronic migraine: a controlled study. *Arq Neuropsiquiatr* 2011;69(4):607–12.
- [25] Fernández-de-las-Heras C, Pérez-de-Heredia M, Brea-Rivero M, Miangolarra-Page JC. Immediate effects on pressure pain threshold following a single cervical spine manipulation in healthy subjects. *J Orthop Sports Phys Ther* 2007;37(6):325–9.
- [26] Aweid O, Gallie R, Morrissey D, Crisp T, Maffulli N, Malliaras P, et al. Medial tibial pain pressure threshold algometry in runners. *Knee Surg Sports Traumatol Arthrosc* 2014;22:1549–55.
- [27] Lunn TH, Kristensen BB, Gaarn-Larsen L, Kehlet H. Possible effects of mobilization on acute post-operative pain and nociceptive function after total knee arthroplasty. *Acta Anaesthesiol Scand* 2012;56(10):1234–40.
- [28] Kosek E, Ekholm J, Nordemar R. A comparison of pressure-pain thresholds in different tissues and body regions. *Scand J Rehab Med* 1993;25:117–24.
- [29] Andrzejewski W, Kassolik K, Brzozowski M, Cymer K. The influence of age and physical activity on the pressure sensitivity of soft tissues of the musculoskeletal system. *J Bodywork Mov Ther* 2010;14:382–90.
- [30] Hogeweg JA, Langereis MJ, Bernards AT, Faber JA, Helder JM. Algometry. Measuring pain threshold. Method and characteristics in healthy subjects. *Scand J Rehab Med* 1992;24:99–103.
- [31] Magora A, Vatine J, Magora F. Quantification of musculoskeletal pain by pressure algometry. *Pain Clinic* 1992;5:101–4.
- [32] Fisher A. Pressure algometry over normal muscles. Standard values, validity and reproducibility of pressure threshold. *Pain* 1987;30:115–26.
- [33] Cimino R, Farella M, Michelotti A, Pugliese R, Martina R. Does the ovarian cycle influence the pressure pain threshold of the masticatory muscles in symptom-free women? *J Orofacial Pain* 2000;14:105–11.
- [34] Isselee H, De Laat A, Bogaerts K, Lysens R. Long-term fluctuations of pressure pain thresholds in healthy men, normally menstruating women and oral contraceptive users. *Eur J Pain* 2001;5:27–37.